



Microbore HPLC: Separation of a Standard Peptide Mixture

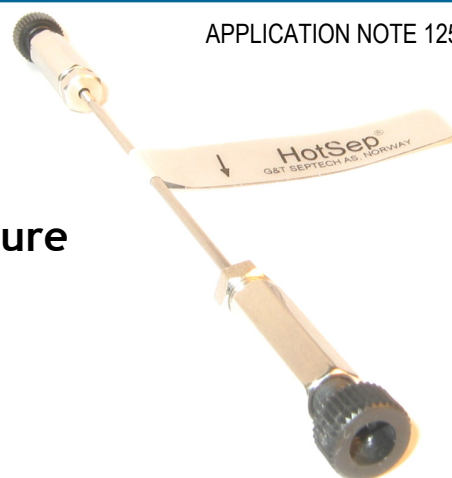

App No 125

Peptides

Column: 3µ ProntoSIL C18 300Å
Dimensions: 1 x 150 mm
Order No.: S-131-1015
Mobile Phase: A: 0.1% TFA in water
 B: MeCN-0.1% TFA in water (70:30)
Gradient: 35 to 80% B in 4 mins
Flow Rate: 50 µL/min
Temp.: 30C
Detector: UV @ 220 nm

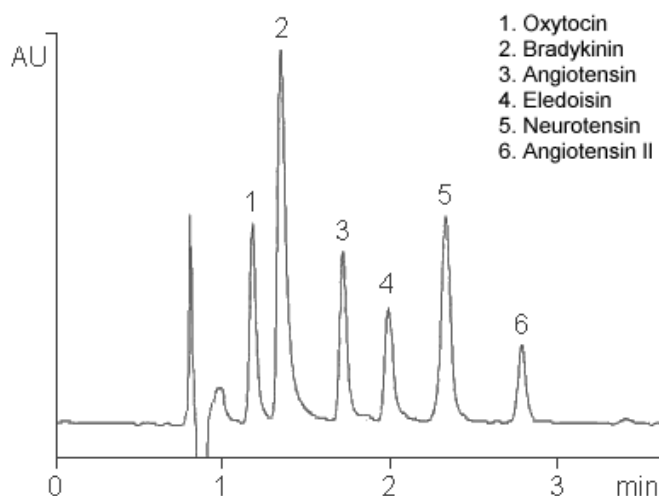

Comments:

Trifluoroacetic acid (TFA) is usually the ion-pairing agent of choice when separating peptides by HPLC-UV.

ORDERING INFORMATION: HotSep® ProntoSIL C18, 3µ, 300Å

ID	3 cm	5 cm	10 cm	15 cm	Guard	Guard/5pk
1.0 mm	S-131-1003	S-131-1005	S-131-1010	S-131-1015	G-131-10-1	G-131-10-5
0.5 mm	S-131-0503	S-131-0505	S-131-0510	S-131-0515	G-131-05-1	G-131-05-5
0.3 mm	S-131-0303	S-131-0305	S-131-0310	S-131-0315	G-131-03-1	G-131-03-5
0.1 mm	---	---	S-131-0110	S-131-0115	---	---
75 µm	---	---	S-131-00710	S-131-00715	---	---