



Microbore HPLC: Hypersil ODS Separation of Xanthines



App No 139

Xanthines

Column: 3 μ Hypersil ODS 100A
Dimensions: 1 x 150 mm
Order No.: S-151-1015
Mobile Phase: MeOH - 50 mM sodium acetate, pH 5 (25:75)
Flow Rate: 50 μ L/min
Temp.: 25C
Detector: UV @ 254 nm

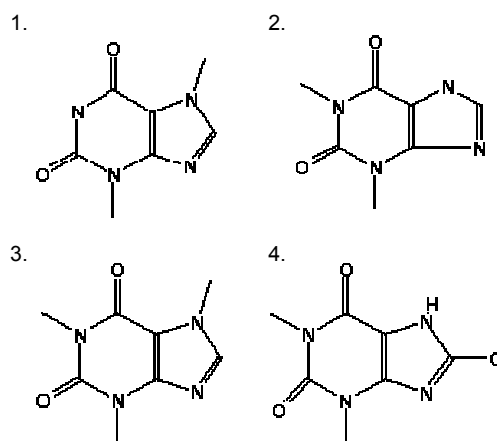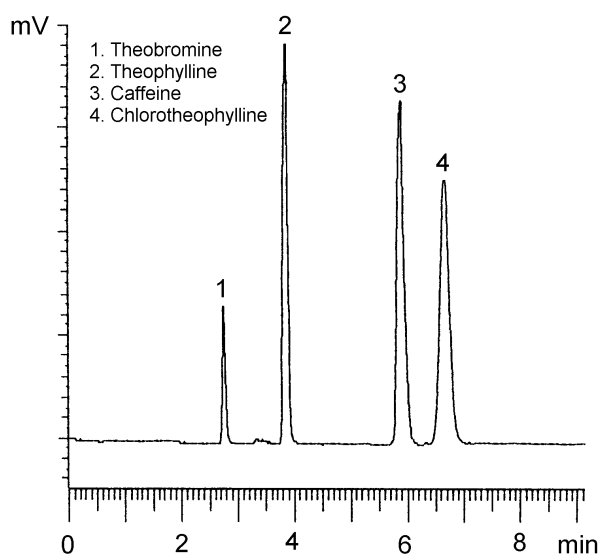

ORDERING INFORMATION: HotSep® Hypersil ODS (C18), 3 μ , 100Å

ID	3 cm	5 cm	10 cm	15 cm	Guard	Guard/5pk
1.0 mm	S-151-1003	S-151-1005	S-151-1010	S-151-1015	G-151-10-1	G-151-10-5
0.5 mm	S-151-0503	S-151-0505	S-151-0510	S-151-0515	G-151-05-1	G-151-05-5
0.3 mm	S-151-0303	S-151-0305	S-151-0310	S-151-0315	G-151-03-1	G-151-03-5
0.1 mm	---	---	S-151-0110	S-151-0115	---	---
75 μ m	---	---	S-151-00710	S-151-00715	---	---